



DC-AIR™ by FTG



incident
Be Inspired

The New Generation of Digital Radiography.

True Wireless with Bluetooth®

The latest in Bluetooth® Low Energy technology enables DC-Air™ to rapidly and reliably transfer clinical images wirelessly to its receiver connected to the PC.

Direct-Conversion Image Quality

Other sensors have to use a component called a scintillator to convert x-ray photons to visible light so they can interpret an image, but not DC-Air™.

Revolutionary direct-conversion x-ray technology converts x-rays directly to electronic signal, creating a more detailed radiograph with better clarity.


Comfort & Convenience

Elimination of cables and patent-pending alignment system minimizes bulk and maximizes ease of positioning.

The sensor can be quickly secured into different positions in each holder for efficient and accurate acquisition of clinical images. The sensor operates with an integrated battery that can be recharged by placing it on the Docking Station.

Built to Last

With its homogenous silicon construction, DC-Air™ is also lighter and more durable than previous generation sensors. It has IP67 dust and water resistance rating, and will stand up to the demands of daily clinical use.

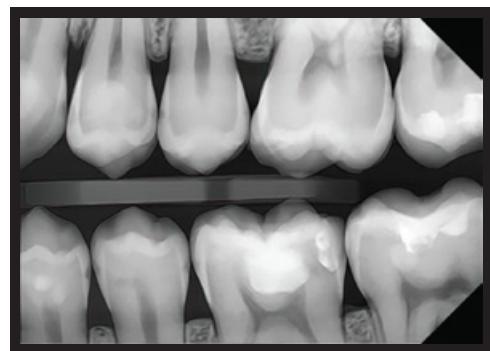

DC-Air™ includes a 2 year warranty and expert imaging support.




© 2021 Freedom Technologies Group
Proudly Manufactured In Finland by Athlos Oy

1 Hellén-Halme, Kristina & Johansson, Curt & Nilsson, Mats. (2016). Comparison of the performance of intraoral X-ray sensors using objective image quality assessment. Oral Surgery, Oral Medicine, Oral Pathology and Oral Radiology, 122, 10.1016/j.oooo.2016.08.014.


Next-generation x-ray technology means better diagnostic clarity.

MTF: The Objective Value for Resolution

The modulation transfer function (MTF) is the spatial frequency response of an imaging system. It is the sharpness at a given spatial frequency. MTF is the most useful measure of true resolution because it accounts for the amount of detail and contrast over a range of spatial frequencies. DC-Air™ achieves a superior MTF value over the full range of diagnostic spatial frequencies for distinctly brilliant image quality.

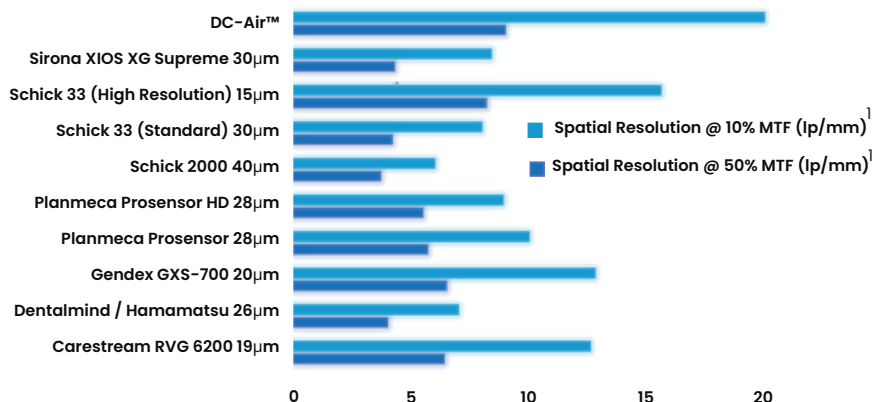

Clinical Images

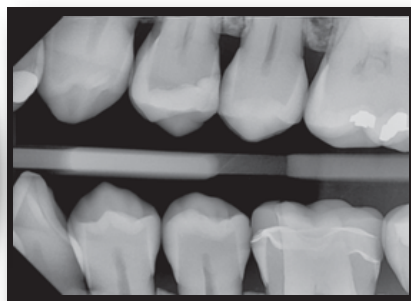

Interfaces

Radio: Bluetooth® Low Energy
Wired: USB 2.0
Connector Type (Docking Station): USB-C
Cable Type (Docking to PC): USB-C to USB Type-A

Technical Specifications

Detector: Single Crystal Direct Conversion Silicon / CMOS
Pixel Size: 26 µm
Exposure Parameters: 0.05 – 0.5 sec, 60 – 70 kV
Active Area: 35.1 mm × 24.7 mm
Pixel Resolution: 12 bits
Number of Pixels: 1,249,920
MTF: >70% @ 5 lp/mm, >40% @ 10 lp/mm

Features

Sensor Mode of Operation: Global Shutter
Triggering: Automatic on X-ray Start
Storage RAM: 4 MB
Images in RAM: 1 Image
Range: Up to 3 m
X-rays per Recharge Cycle (Continuous Use): 150+

Sensor Battery

Type: Lithium-Ion
Capacity: 19 mAh


Docking Station Power

Input Voltage: +5V ± 10%
Input Power (Max): 2.5 W

Environmental

Ambient Operating Temperature: +50°F to +95°F
Transportation Temperature: -4°F to +122°F
Long-Term Storage Temperature: +32°F to +95°F
Humidity (Non-Condensing): 30% – 95%

Hardware Dimensions

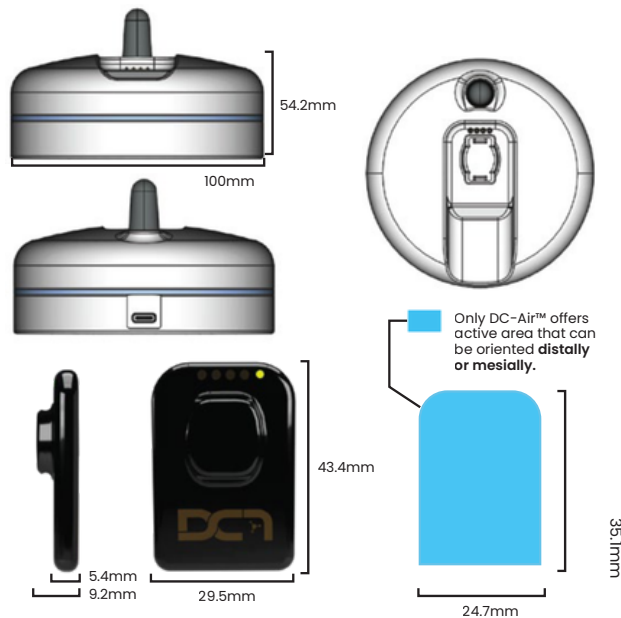

Contact Us:
+91 70459 30935 | info@indentindia.com
www.indentindia.com